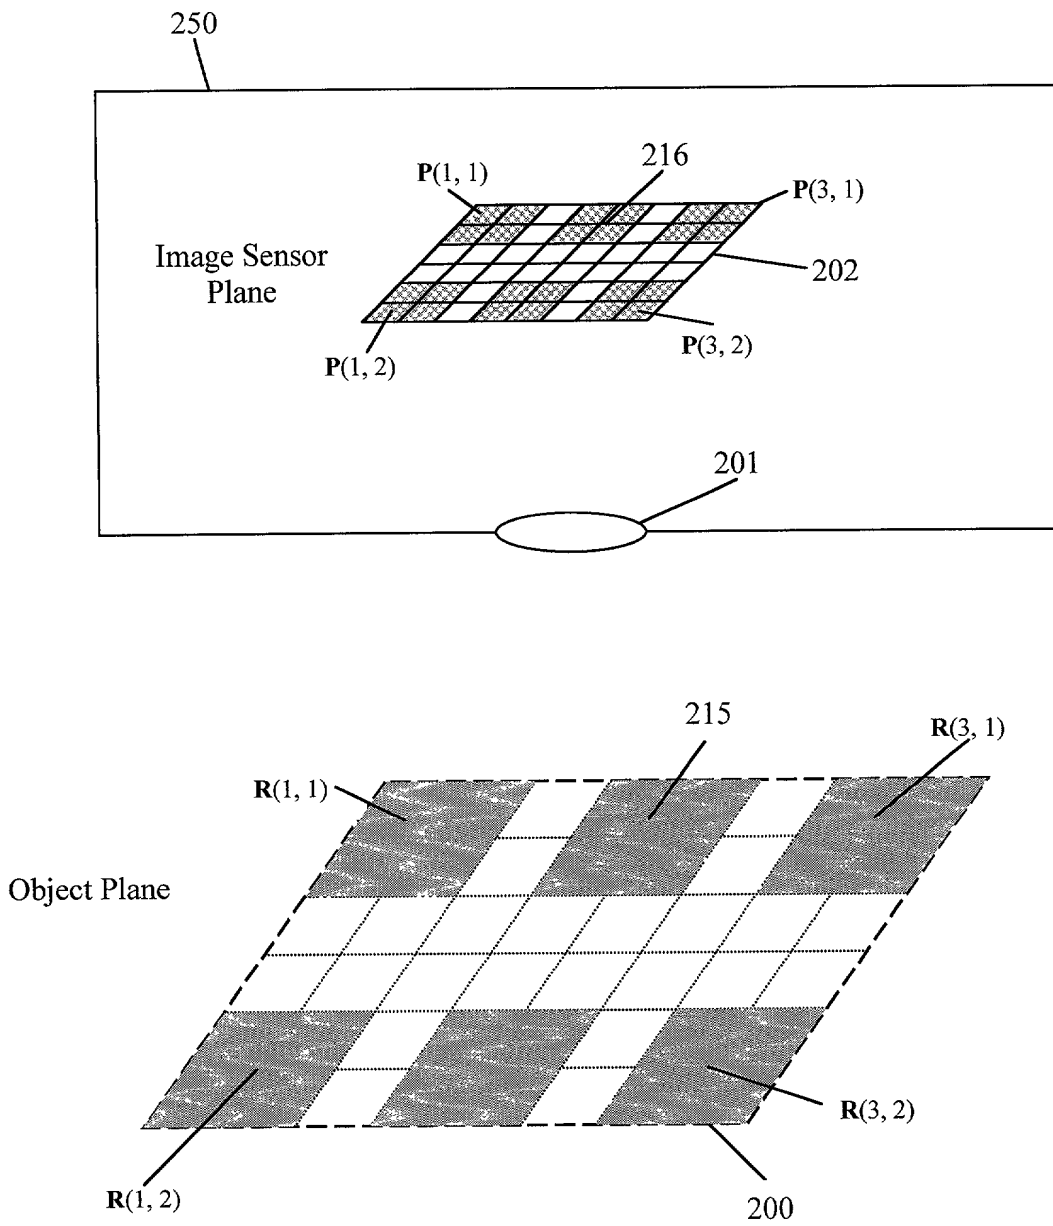
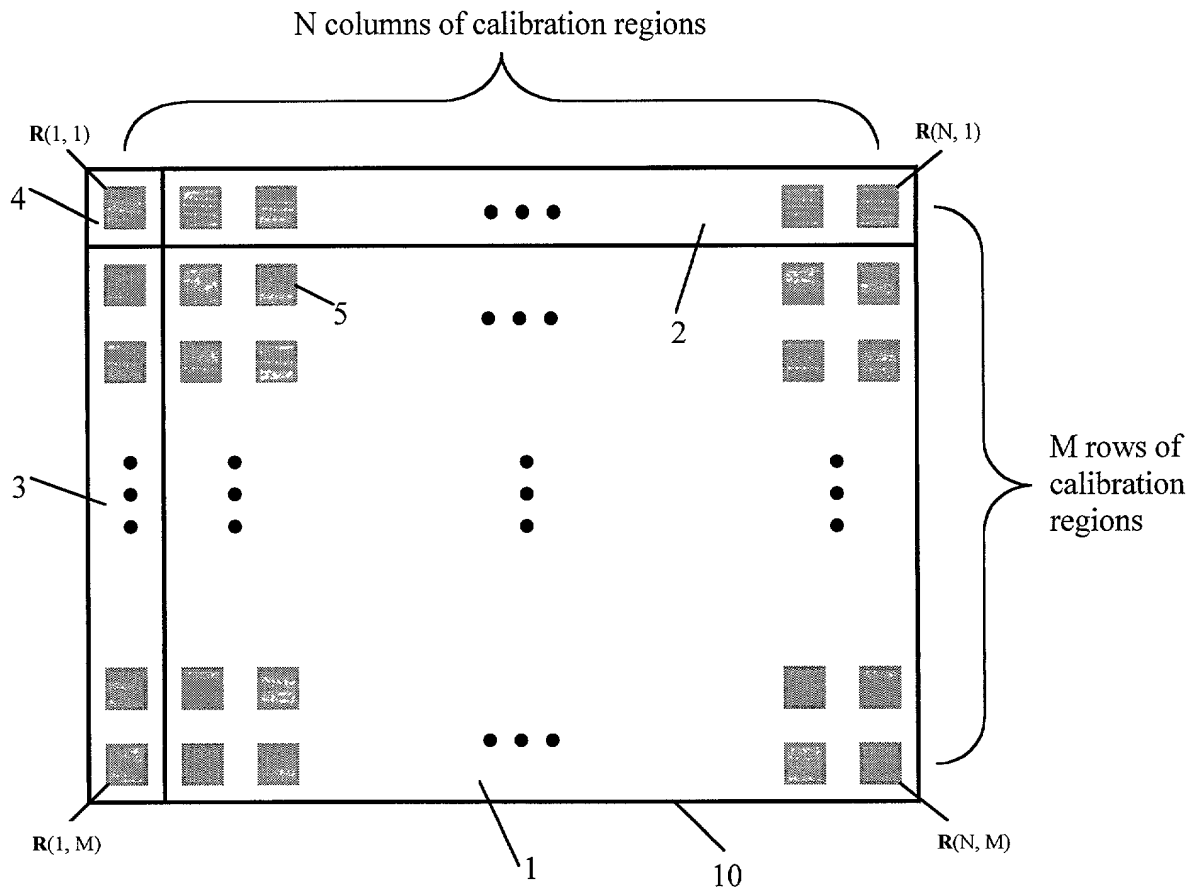



Figure 1



**Figure 2**



**Figure 3**

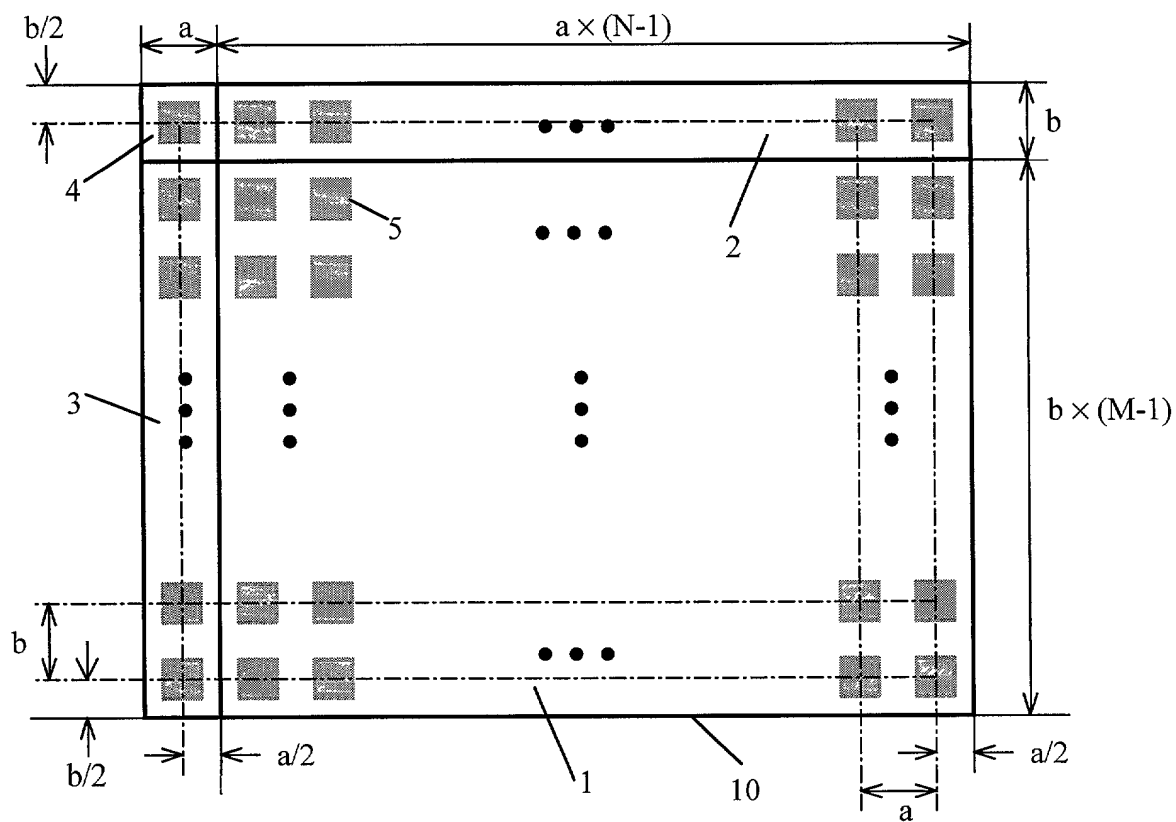

- a: horizontal interval of calibration regions  
b: vertical interval of calibration regions

**Figure 4**

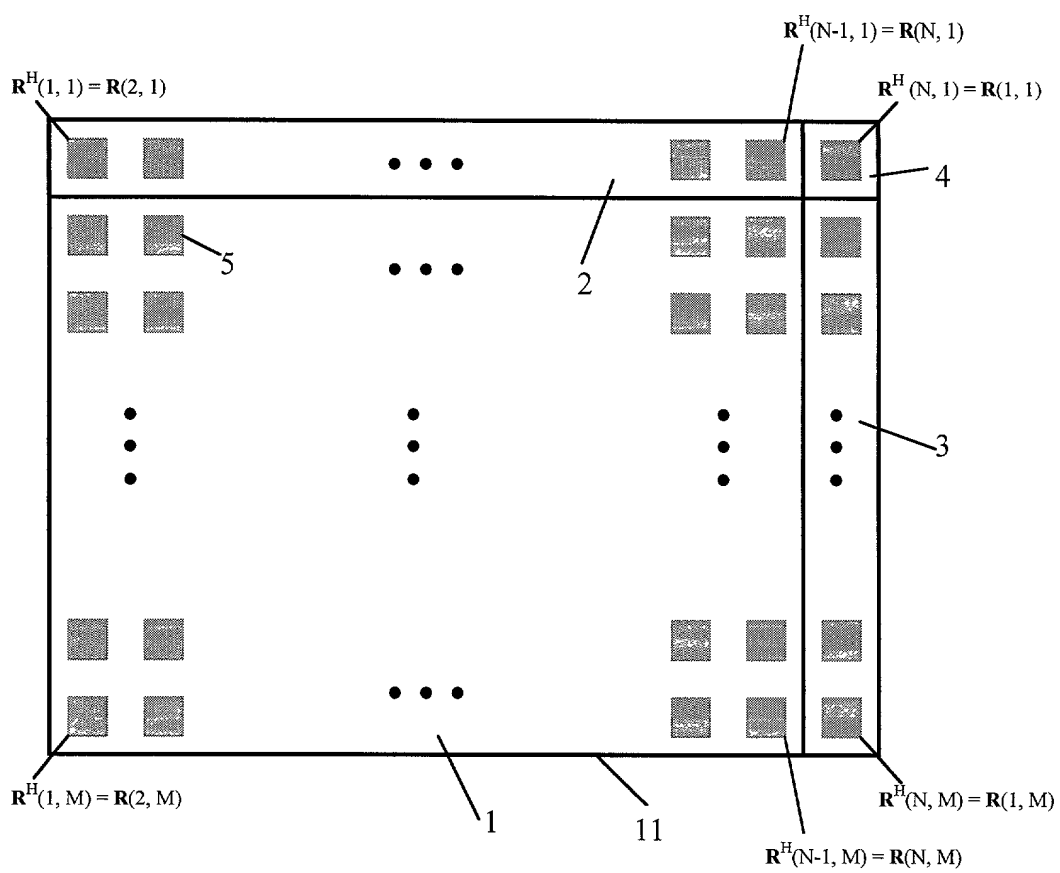


Figure 5

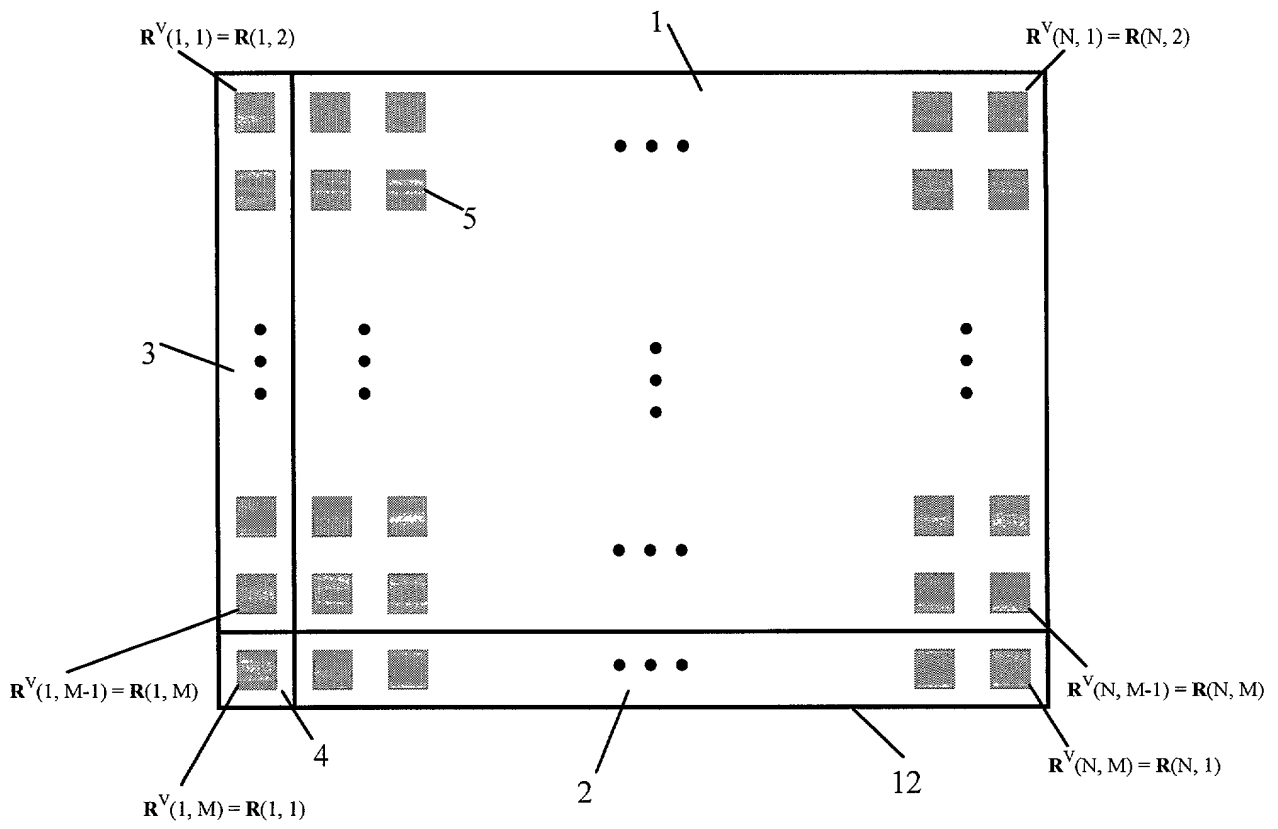
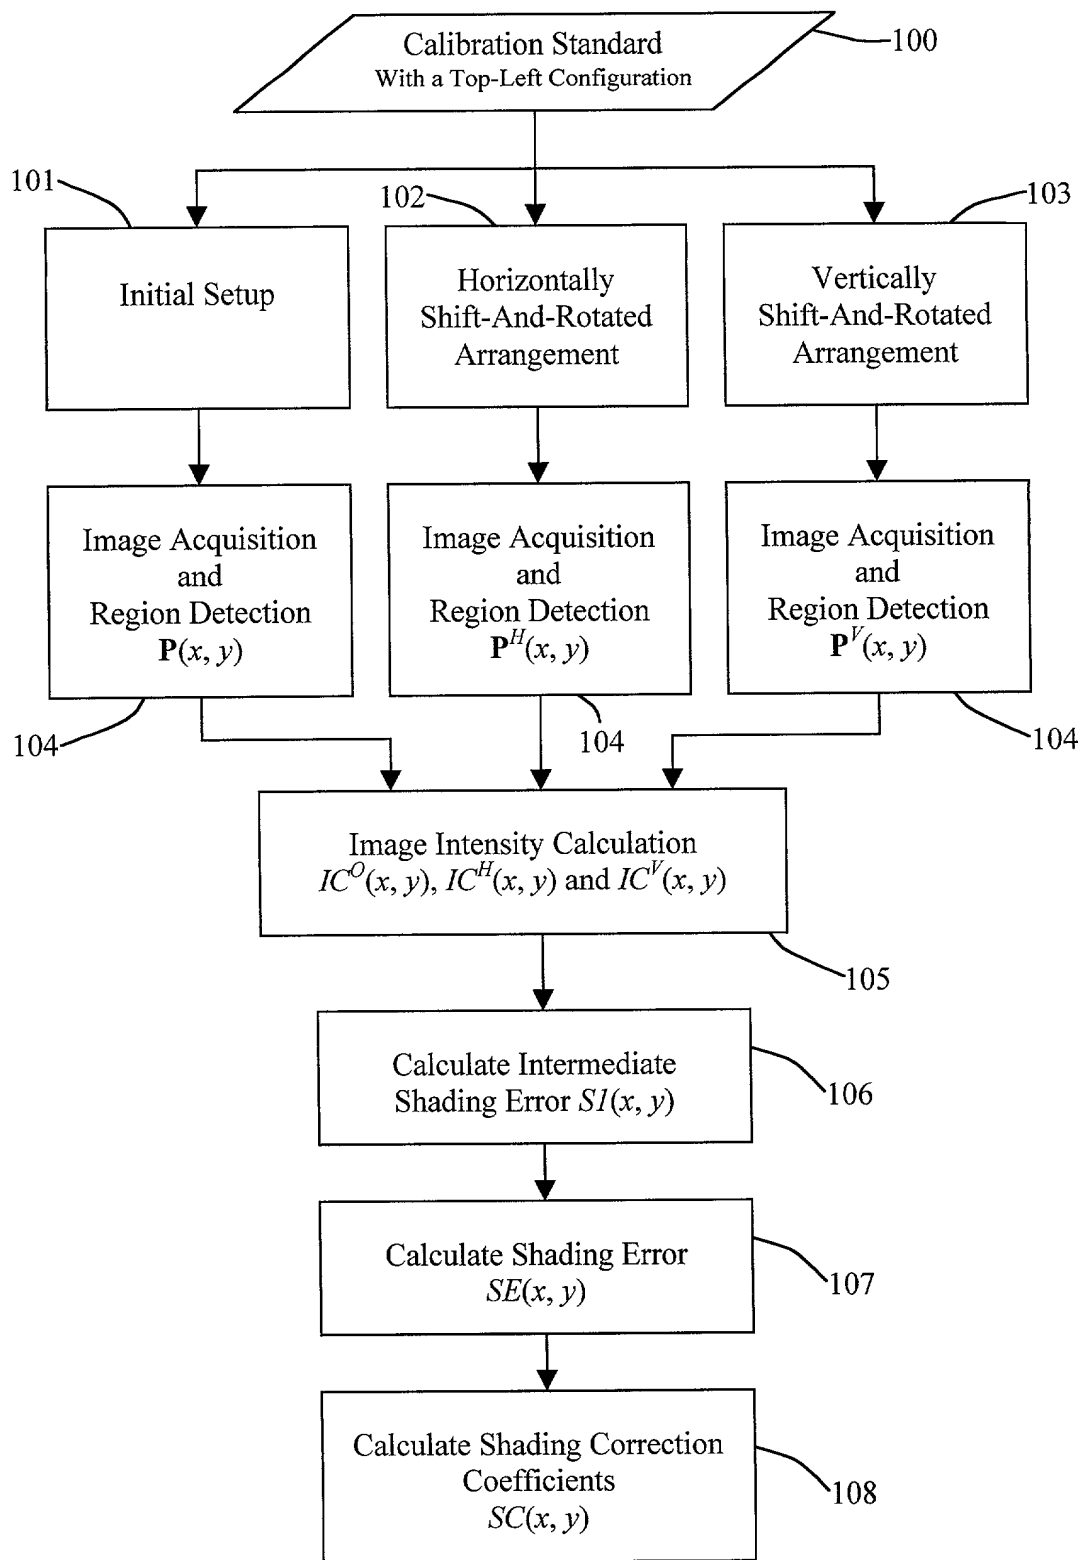
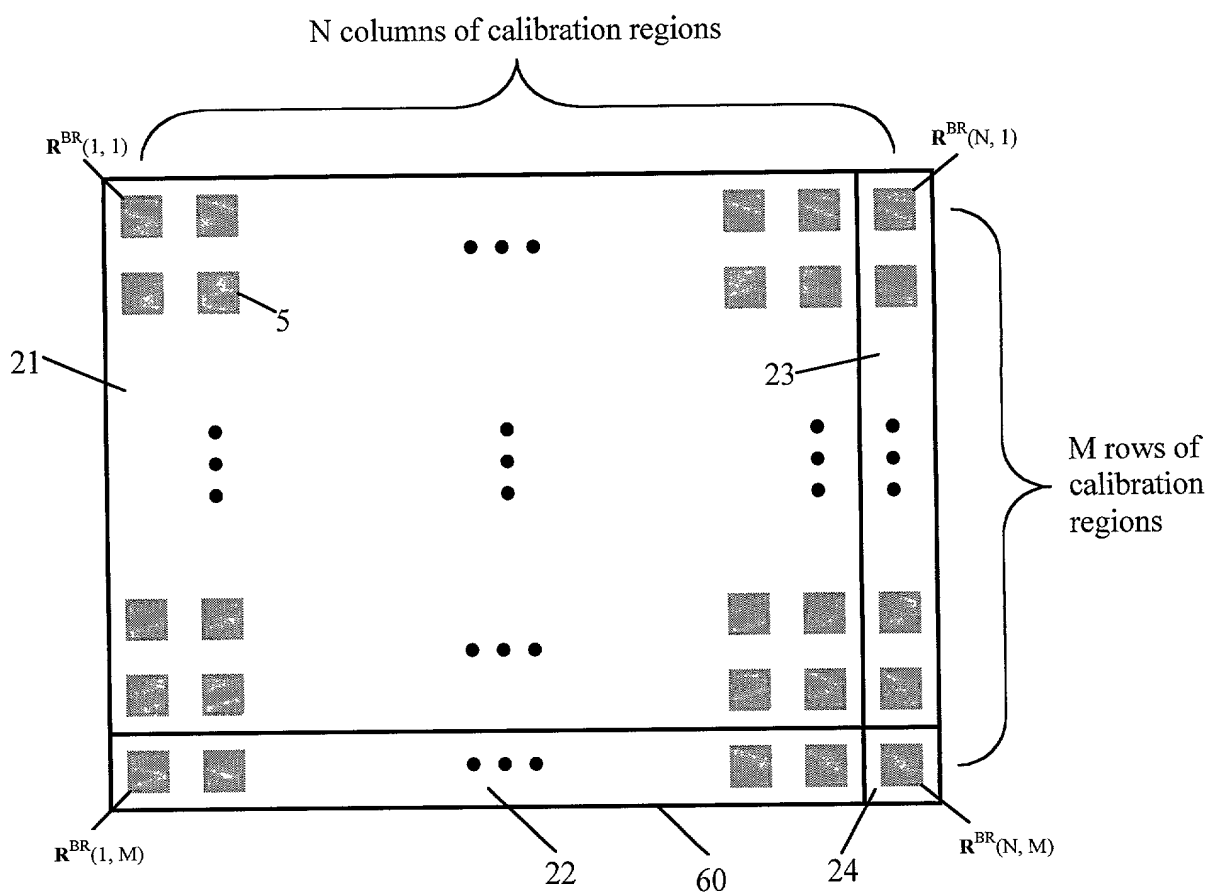


Figure 6



**Figure 7**



**Figure 8**



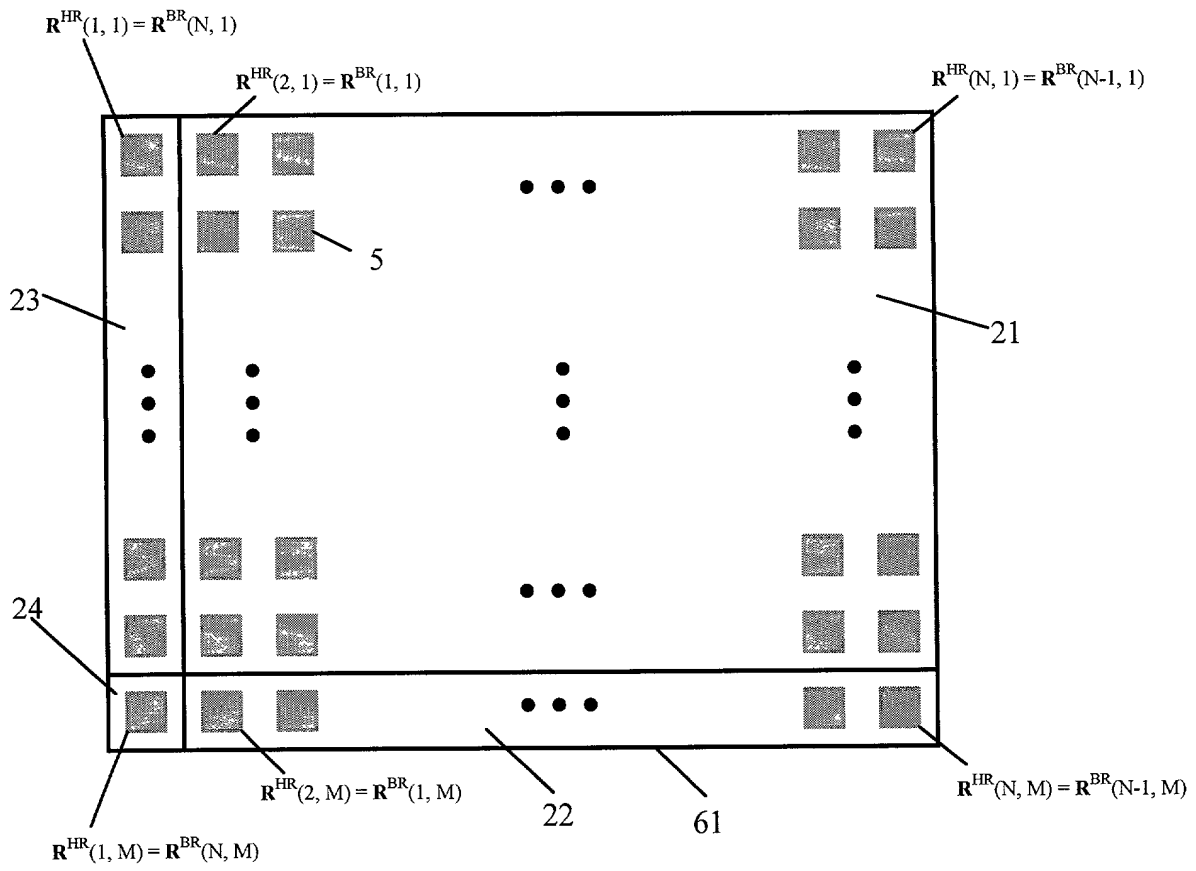


Figure 9

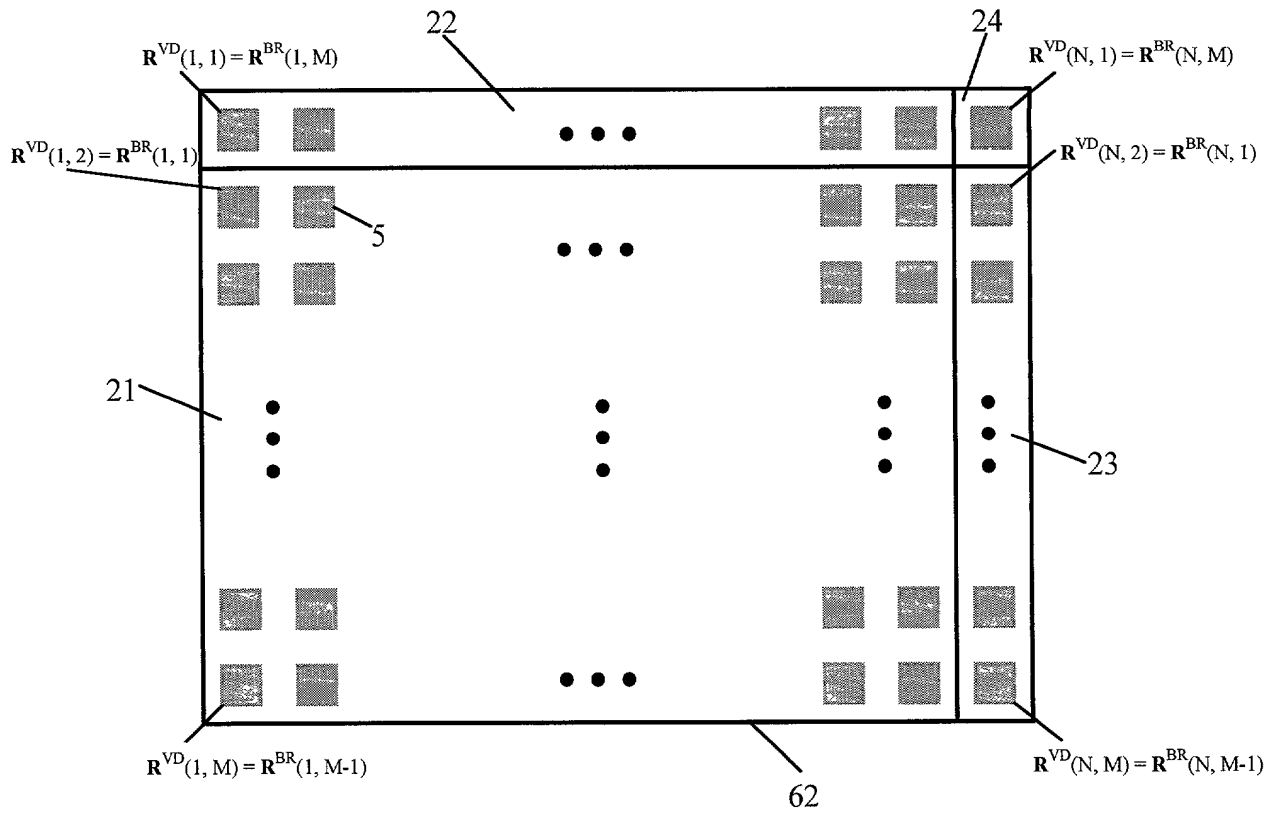
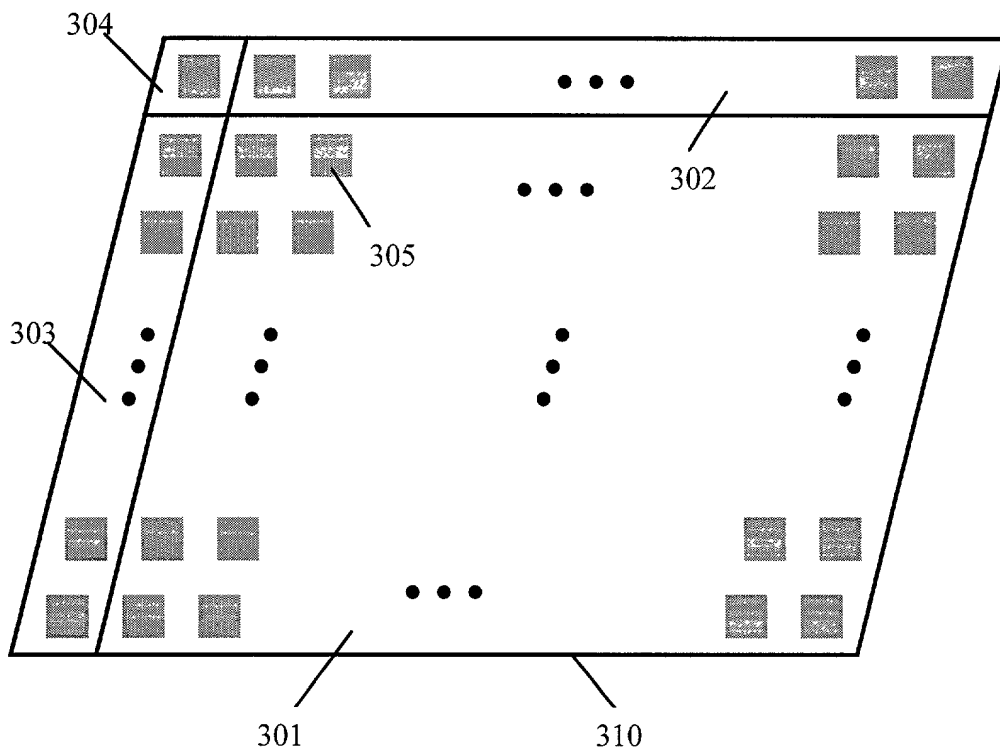


Figure 10



**Figure 11**

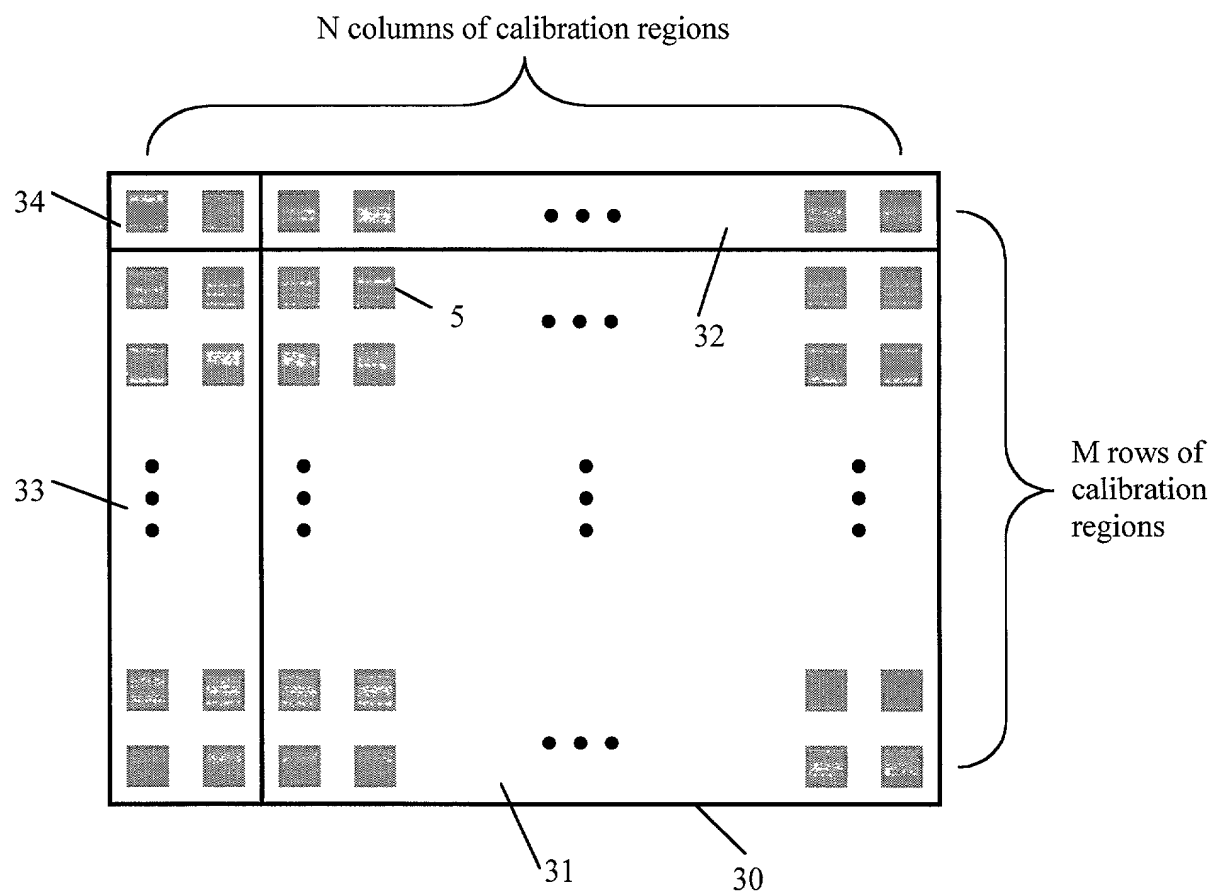


Figure 12

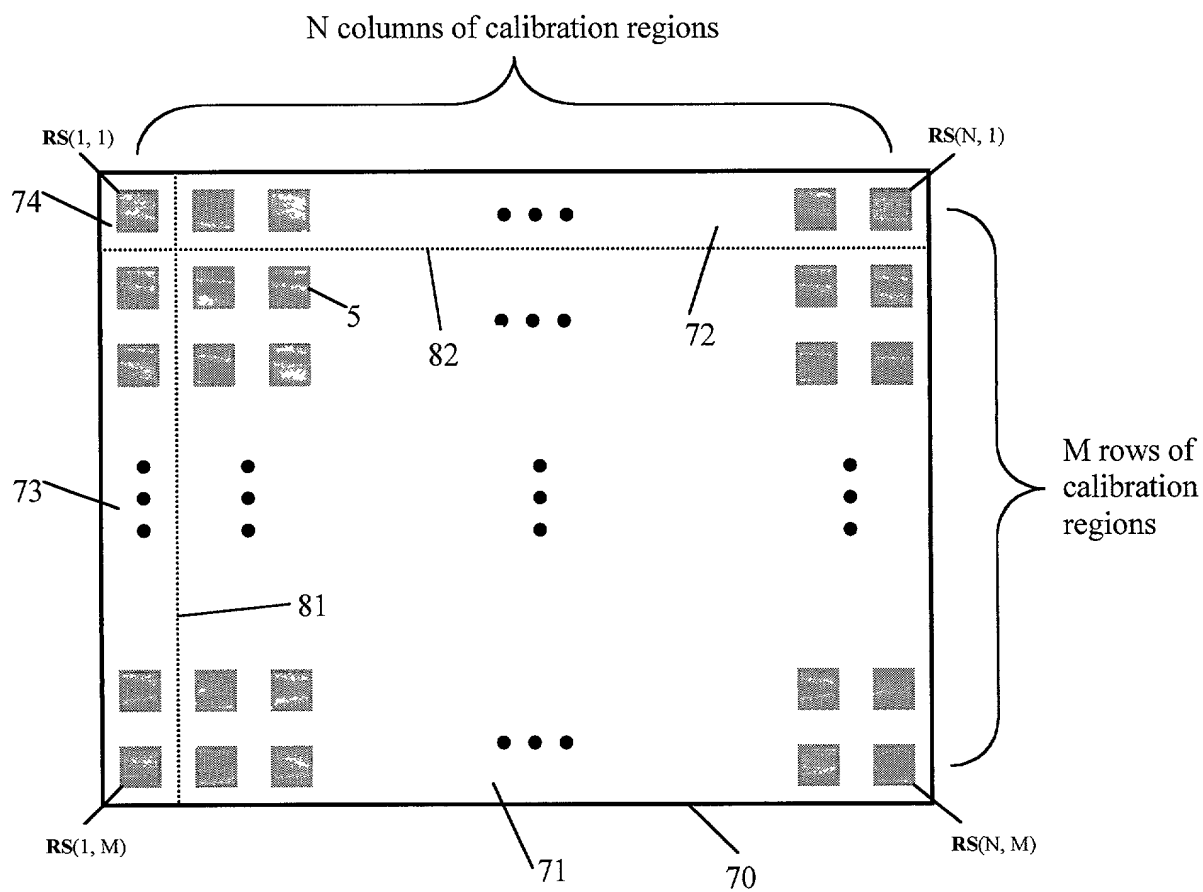


Figure 13

Shift the standard left 1 column and image

Shift the standard right N-1 columns and image

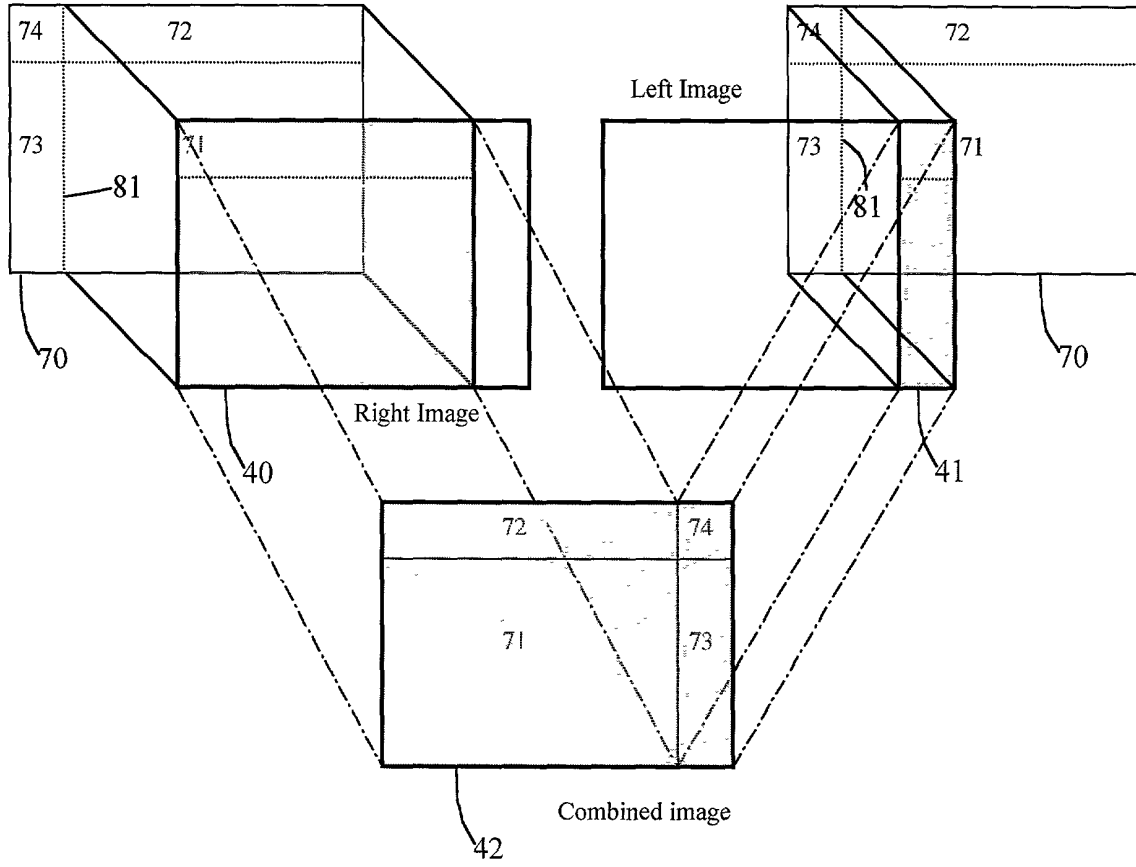



Figure 14

[illegible][illegible][illegible]

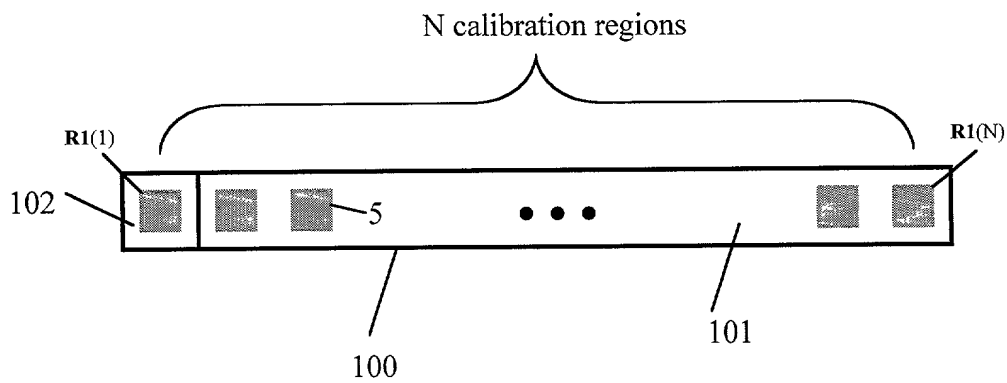


Figure 16

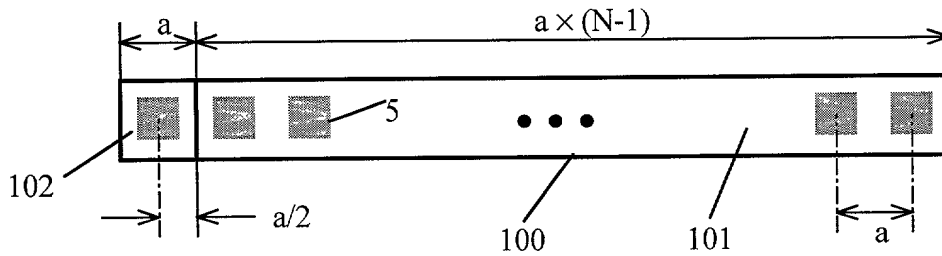


Figure 17

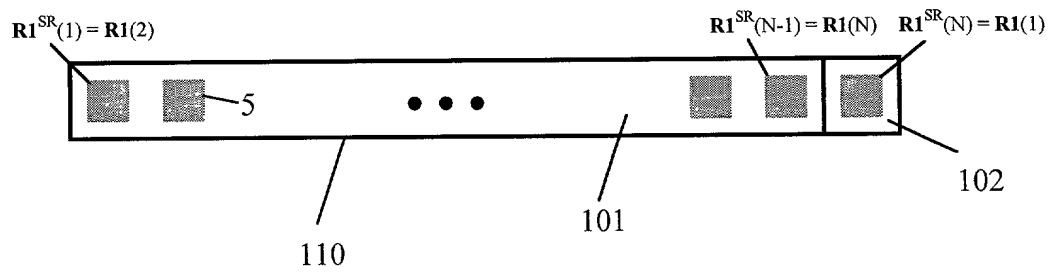


Figure 18



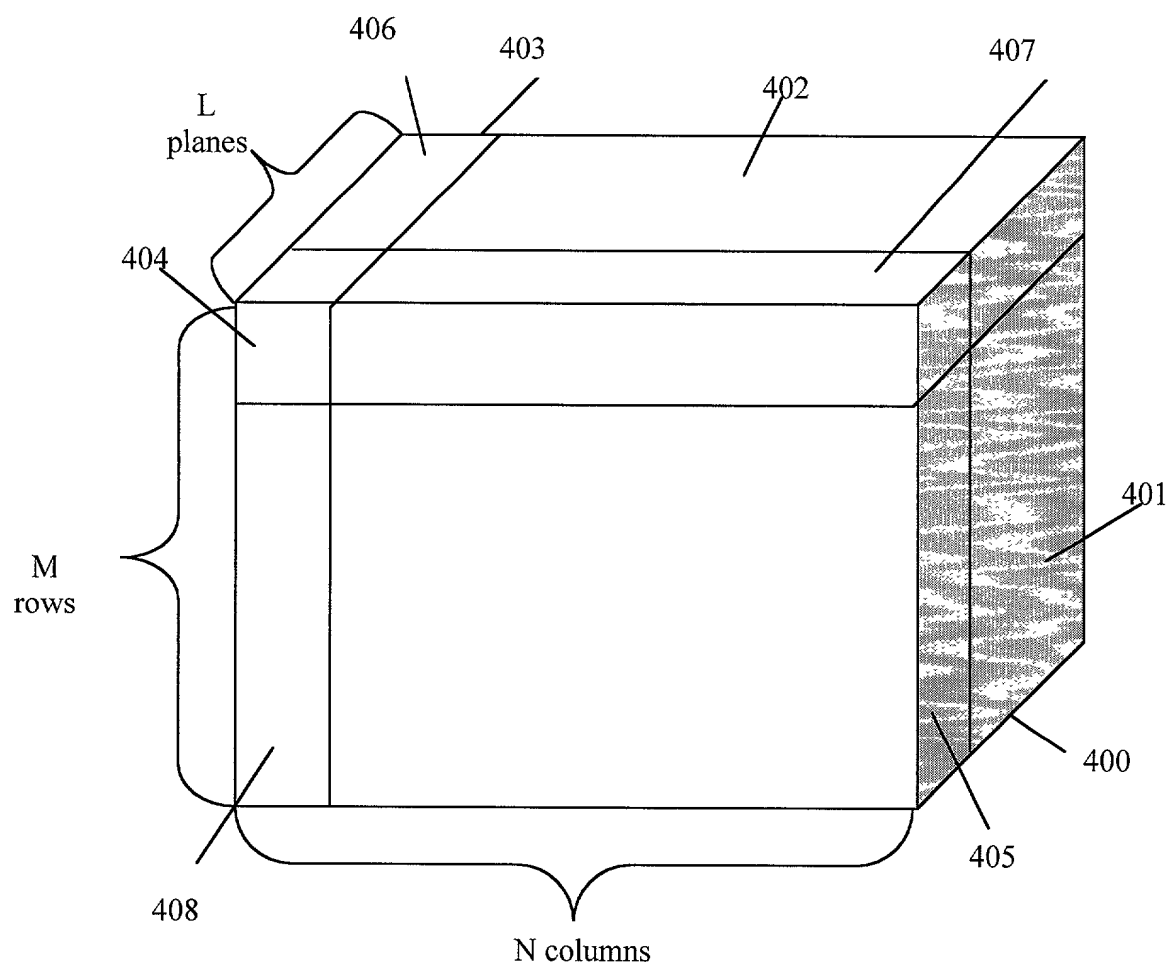


Figure 19